CODONICS Disinfection Technology™

D7000

Quick Set Up Guide

Step 1 - Unpack the Codonics Disinfection Technology (CDT) D7000 by opening the top of the box. Lay the box on its side with the corrugated slider down as shown in Step 2. It is recommended that two people unpack the D7000 as it is solidly built and heavy.

Step 2 - Slide the D7000 out, vertically stand the unit up and remove the protective foam packaging materials. Place the D7000 on a solid, level surface on its bottom end with Mounting Stand as pre-assembled from the factory.

Step 3 - Unpack the D7000 Cartridge and Power Cord (not shown).

Place the D7000 Cartridge on a solid, level surface until it is ready to be installed into the system per Step 5.

Step 4 - Turn the D7000 for access to the rear panel. The AC input module on this device has been set for the voltage range for your power usage. Ensure the voltage range is set properly by the raised numerals pointing to the Applied Voltage Arrow on right side of socket. See the CDT User's Manual for more info.

Step 5 - Turn the D7000 for access to the Front Panel. Push the Open button and pull the drawer upwards. Holding the yellow handles, align the Cartridge with the two metal vertical pins and push down to interlock it with the white electronics connector.

Step 6 - Place the D7000 in the area intended for use.

Refer to the CDT User's Manual for location and placement warnings and precautions.

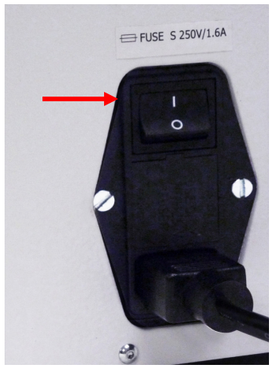

Step 7 - The Power Cord is factory connected to the Power Input Port. Connect the Power Cord to a grounded power outlet that supplies the appropriate voltage for your specific region of the world. Turn the D7000 on with the Power Switch by placing it into the "I" position as shown. After five (5) seconds, the System LED light will flash in green and the system operations (fans) will be audible.

Step 8 - After thirty (30) seconds, the system warm up process will be completed. The System LED and Cartridge LED lights will be solid green.

With those indications, the D7000 is ready for use.

Codonics Disinfection Technology D7000 Quick Set Up/Reference Guide
Copyright © 2013 - 2014 by Daylight Medical, Inc. All rights reserved, worldwide. Printed in the USA. Part Number 900-667-001.

CODONICS Disinfection Technology™

D7000

Quick Reference Guide

Step 1 - Place the mobile device face (screen) back into the Entry Slot of the D7000 Front Panel.

If an optional CDT Disinfection Sleeve is used, place into the Entry Slot with the sleeve closure (zip or flap) on the leading (front) end.

Step 2 - The D7000 sensors detect the entry of a mobile device and activate the transport rollers, which will feed the device through the Cartridge's two high-output ultraviolet C (UVC) bulbs utilized for the disinfection process.

Step 3 - The D7000 will disinfect the mobile device.

On average, a mobile device the size of an iPad® will be processed for disinfection in twenty-five (25) seconds.

Step 4 - When the disinfection process is completed successfully, the mobile device will be lowered into the Exit Compartment for retrieval and the Check Mark LED on the D7000 Front Panel will flash in green.

Step 5 - The disinfected mobile device is now ready for use and can be taken into medical settings where infection prevention is desirable.

Step 6 - If an optional CDT Disinfection Sleeve is desired for usage, locate the appropriate sized sleeve for your mobile device.

One single or two nested sleeve options are available for use.

Step 7 - Slip the mobile device into the sleeve(s) and close each sleeve by using the zip(s) or the adhesive strip(s) on the sleeve flap and process per Step 1. Note: If marker is present, the white portion of the sleeve marker is blank. (A check mark will be visible upon a completed disinfection cycle).

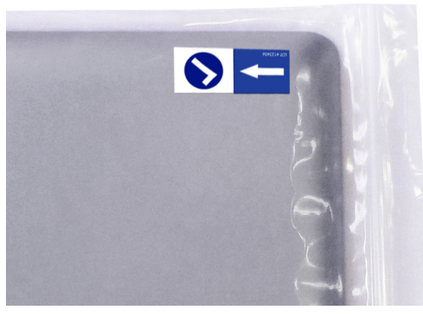

Step 8 - The disinfected mobile device is lowered into the Exit Compartment.

Note: If the marker option was chosen, the sleeve marker will now show a visible check mark. The mobile device is now ready to be picked up by the user.

Codonics Disinfection Technology D7000 Quick Set Up/Reference Guide
Copyright © 2013 - 2014 by Daylight Medical, Inc. All rights reserved, worldwide. Printed in the USA. Part Number 900-667-001.